MKS

Instruction Manual

114103 - P1
REV B, 7/92

MKS Type 690 Absolute
MKS Type 698 Differential
High Accuracy Pressure Transducers

SIX SHATTUCK ROAD, ANDOVER, MASSACHUSETTS 01810 (508) 975-2350 (800) 227-8766 FAX (508) 975-0093

MKS INSTRUMENTS, INC.

WARRANTY

for Type 690 and 698 Equipment

MKS Instruments, Inc. (**MKS**) warrants that the equipment described in the face of this warranty (the "equipment") manufactured by **MKS** shall be free from defects in materials and workmanship for a period of two years from date of shipment. For the period commencing with the date of shipment of this equipment and ending two years later, **MKS** will, at its option, either repair or replace any part which is defective in materials or workmanship without charge to the purchaser. The foregoing shall constitute the exclusive and sole remedy of the purchaser for any breach by **MKS** of this warranty.

The purchaser, before returning any equipment covered by this warranty, which is asserted to be defective by the purchaser, shall make specific written arrangements with respect to the responsibility for shipping the equipment and handling and other incidental charges with the **MKS** sales representative or distributor from which the equipment was purchased or, in the case of a direct purchase from **MKS**, with the **MKS** home office in Andover, Massachusetts, U.S.A.

This warranty does not apply to any equipment which has not been used in accordance with the specifications recommended by **MKS** for the proper and normal use of the equipment. **MKS** shall not be liable under any circumstances for consequential or incidental damages in connection with, or arising out of, the sale, performance, or use of the equipment covered by this warranty.

THIS WARRANTY IS IN LIEU OF ALL OTHER WARRANTIES BY **MKS**, EXPRESS OR IMPLIED, INCLUDING THE IMPLIED WARRANTY OF MERCHANTABILITY, THE IMPLIED WARRANTY OF FITNESS FOR A PARTICULAR PURPOSE, AND ANY WARRANTY AGAINST INFRINGEMENT OF ANY PATENT.

3-93 114103-P1

114103-P1
REV B 7/92

MKS Type 690 Absolute
MKS Type 698 Differential
High Accuracy Pressure
Transducers

Copyright © 1992 by MKS Instruments, Inc.

All rights reserved. No part of this work may be reproduced or transmitted in any form or by any means, electronic or mechanical, including photocopying and recording, or by any information storage or retrieval system, except as may be expressly permitted in writing by MKS Instruments, Inc.

TABLE OF CONTENTS

1. TYPE 690/698 TRANSDUCERS

1-1 GENERAL 1-1

1-2 FUNCTIONAL DESCRIPTION 1-1

1-3 SPECIFICATIONS 1-3

1-4 INSTALLATION 1-5

1-5 START-UP/OPERATION 1-8

1-6 TROUBLESHOOTING 1-11

1-7 MAINTENANCE 1-12

2. TYPE HS-1 TRANSDUCER SIMULATOR

2-1 DESCRIPTION 2-1

2.2 OPERATING INSTRUCTIONS 2-2

Digitized by the Internet Archive
in 2026

https://archive.org/details/manualsplus_11999

1. 690/698 HIGH ACCURACY PRESSURE TRANSDUCERS

1-1 GENERAL

This manual describes the MKS-690 Series (Absolute) and 698 Series (Differential) Baratron[R] Pressure Transducers.

These transducers, when used with their required MKS Type 270 Signal Conditioner/Readout or MKS Type 170M-6 Signal Conditioner, represent the best pressure measurement system (sensor/transducer, signal conditioner, digital readout) currently produced by MKS. For further information on the companion Signal Conditioner/Readouts, please refer to the 270 or 170M-6 instruction manuals.

These precision pressure measurement systems are available with high basic accuracies, wide dynamic range, and a typical Zero Coefficient of 1-2 ppm/°C and a Span Coefficient of 10-15 ppm°C (higher for the 100 mTorr range).

1-2 FUNCTIONAL DESCRIPTION

The 690/698 Baratron[R] is composed of four (4) sub-sections assembled within a precision die-cast housing. These are: 1) an Inconel variable capacitance diaphragm sensor; 2) an electronic preamplifier and bridge circuits; 3) an inner temperature control housing; 4) a P.C. Board. The all Inconel sensor, together with its high impedance bridge circuit and preamp, is mounted within a thick-walled, temperature-controlled aluminum housing. This miniature "environmental chamber" reduces the ambient temperature effects upon the sensor and bridge circuit by more than a factor of 50.

The main P.C. Board mounted outside the temperature-controlled housing consists of those circuits necessary to convert a low level 10 KHz signal to a precise 1/4 V/V output that is linearly proportional to pressure. Also, that circuit necessary to maintain the housing temperature is located on this board. All gain controlling components are selected for maximum stability (wire-wound resistor, NPO capacitor, etc.). A "system check" circuit is used which will point out any gain change experienced at any point in the electrical system.

Baratron[R] is a Registered Trademark of MKS Instruments, Inc.

The 690 Baratron® is able to make a reliable absolute pressure measurement by virtue of its own built-in "zero" pressure reference cavity. During production, the low pressure side (P_R) of the sensor is pumped to less than $1x10^{-7}$ mmHg, outgassed thoroughly, chemically gettered, and permanently sealed. The extremely low gas loads and active gettering material in the reference cavity assure the user of many years of useful service.

The 698 Baratron® is unique, in that the entire differential sensor is surrounded by an Inconel case. Ambient line pressure (P_R) appears between the sensor and this case, thus eliminating sensitivity changes due to line pressure induced stress variations within the sensor structure. Careful deadweight testing has shown a variation of less than .01% of reading as the line pressure varies from 1 to 15 psiA.

1-3 SPECIFICATIONS

Sensor Model Number	690	698
Type of Measurement	Absolute	Differential, Gauge
Sensor Type	Single-Sided	Single Sided
Measurement Side (P_X) Media Compatibility	Any gas compatible with Inconel, 304SS	Any gas compatible with Inconel, 304SS
Volume (P_X)	2 cc	2 cc
Reference Side (P_R) Media Compatibility	Not applicable	Any dry gas compatible with Inconel, 304/306SS Fosterite, Palladium
Ref. Side Volume	Not Applicable	8cc
Inlet Tube Fitting/s	Cajon® 4VCR (female) orbitally butt welded.	Cajon® 4VCR (female) orbitally butt welded.
Accuracy	STD: 0.08% of Reading ± zero/span coeff.	STD: 0.08% of Reading ± zero/span coeff.
	OPT: 0.05% of Reading ± zero/span coeff.(1)	OPT: 0.05% of Reading ± zero/span coeff.(1)
	OPT: 0.12% of reading ± zero/span coeff.	OPT: 0.12% of reading ± zero/span coeff.
	OPT: 0.02% of reading ± zero/span coeff.(2)	OPT: 0.02% of reading ± zero/span coeff.(2)
Temperature Effects on Zero	<4ppm, FS/°C (Temp controlled @ 45°c) <25 PPM, FS/C (Temp control'd @ 45°c).(3) (0.12% of R Accuracy: <15PPM, FS/°C) (Temp controlled @ 45°C)	<4ppm, FS/°C Temp controlled @ 45°c) <25 PPM, FS/C (Temp control'd @ 45°c.(3) (0.12% of R. Accuracy: <15PPM, FS/°C) (Temp controlled @ 45°C)
Temp Effects on Span	<0.002% R/°C <0.010% R/°C (3)	<0.002% R/°C <0.010% R/°C (3)
Ambient Temperature Operating Range	15-40°C (40°C Maximum)	15-40°C (40°C Maximum)
Pressure Ranges Available (F.S.)	.1, 1, 10, 100, 1000, 5,000, 10,000, 20,000, 25,000 Torr	.1, 1,10,100,1000 Torr

(1) 0.05% available only on .1,1,10,100 and 1000 mmHg units.
(2) Available with L.O. option.
(3) For 100 mTorr only.

1-3 SPECIFICATIONS (Continued)

Sensor Model Number	690	698
Usable Resolution	5 Decades	5 Decades
Px Overpressure	125% F.S. or 45 psia (whichever is greater)	125% F.S. or 45 psia (whichever is greater)
	125% F.S. or 40 psia[1] (whichever is greater)	125% F.S. or 40 psia[1] (whichever is greater)
Maximum Line Pressure	N/A	150 psi
Line Pressure Effects on Span	N/A	<.010%/15 psi[1]
Time Constant With		
270 in Fast Position	<25 ms	<25 ms
Std Position	40 ms	40 ms
Slow Position	400 ms	400 ms

DIMENSIONS

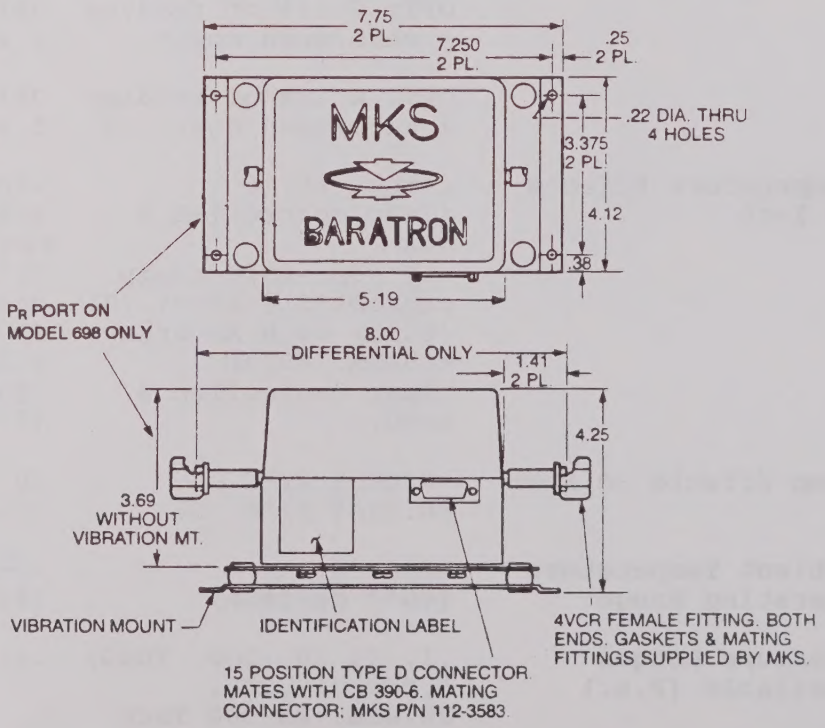

[1]For 100mTorr only

Cajon[R] is a Registered Trademark of the Cajon Company

1.4 INSTALLATION

The Type 690/698 transducer may be mounted horizontally upon its vibration isolation base with the following points noted:

A. All units are supplied with vibration isolators which should be used for maximum stability. A flexible bellows connection is suggested to minimize vibration. Furthermore, it is recommended that the sensor be mounted such that the sensor diaphragm plane is parallel to the major axis of vibration (diaphragm plane is perpendicular to port axis).

B. Ambient temperature around the 690/698 transducer must not rise above 40°C as this will cause the 45-47°C control temperature to go out of regulation, thus destroying the system stability.

C. Mount the transducer as far from RFI and EMI sources as possible. Field experience has shown that care in positioning the transducer initially will prevent future difficulties. The MKS system is internally protected against RFI and EMI. However in a system where several ground potentials are possible, a noisy environment may cause output to be unstable. When this happens, we have found the only solution has been an examination and correction of the source of RFI/EMI.

   Example:

   An SCR supply used in some systems should have the power-carrying wires that run to the chamber twisted to cancel high frequency magnetic fields. Never run the 690 to Signal Conditioner cable in the same wiring bundle as RF or SCR signals.

D. If a dirty pressure medium is expected, mount the sensor with port facing down so that dirt will not fall onto the diaphragm.

E. Connection cables are as follows:

   690/698 to 170M-6C = CB-690-6
   690/698 to 170A/B = CB-270-2-10

F. The vibration mount assembly is shipped from MKS with two shipping screws in place. For noise-free operation, these screws must be removed. However, when this Baratron is subsequently reshipped on a piece of equipment, these screws MUST BE REINSTALLED as the rubber feet will withstand no more than 3 g's force in transit.

G. When installing a 698 Differential Transducer, allow for a cross-porting manifold; i.e. connecting the two ports together. In order to properly set the zero of any differential sensor, there must be equal pressure on both sides of the sensor.

H. Vacuum Connections: The sensor should be connected to the vacuum system via an appropriate isolation valve and bellows tubing.

a. To maximize the life and zero repeatability of the sensor, an isolation valve should be used. Set its closing point at or slightly above the transducer's full scale range.

An isolation valve serves to protect the sensor in two ways:

First: from overpressure, which is common in processing systems that incorporate pressure purging cycles in excess of sensor specifications.

690 Absolute	125% of F.S. or 45 psia (whichever is greater).
698 Differential	125% of F.S. or 45 psia (whichever is greater).
	(Lower for 100mTorr Range)

Second: from contamination by moisture, which is present when a process system is vented to atmosphere. Moisture can often combine with residue on the sensor and/or system surfaces, and form acids such as HCL when Chlorine - based processes are used.

Any good quality electric, or air-operated valve, such as a Nupro® Type 4BK or MKS P/N 108818, or equivalent, is recommended.

b. The sensor inlet should be connected to the isolation valve via an appropriate length of stainless steel bellows tubing with welded mating Cajon® fittings. Both VCR fittings and flexible tubing are products of the Cajon Company.

The use of a flexible bellows completes vibration isolation to the sensor, allowing it to function independently of significant system vibration or stress that could be induced during operation or shipment.

```
* * * * * * * * *  CAUTION  * * * * * * * * * *
*  Hard coupling of the sensor inlet tube so  *
*  that the transducer is suspended by this   *
*  tube is not recommended as the weight of   *
*  the entire assembly will cause stress on   *
*  the sensor.                                *
* * * * * * * * * * * * * * * * * * * * * * * *
```

c. 698 Differential Sensors: The P_X port must be connected to the high side of any system whose differential pressure is to be measured. The P_R side will then be connected to the low pressure side. If connections are reversed, the instrument will output a negative signal whose accuracy is not specified. A 698 Differential sensor may be used to make an absolute measurement, by continually pumping the P_R port to a pressure below that of the resolution of the sensor. (Example: 1mmHg F.S. x 10^{-6} = $<10^{-6}$ mmHg).

```
* * * * * * * * *  CAUTION  * * * * * * * * * *
*  Do not attempt to change the inlet tube    *
*  fitting by cutting or welding.  If a       *
*  different fitting is desired, make up an   *
*  adaptor, or consult MKS for a quotation    *
*  on a special-version sensor.               *
* * * * * * * * * * * * * * * * * * * * * * * *
```

For your convenience, MKS makes available several lengths of these bellows assemblies, including the mating VCR fittings welded to the bellows tubing. To order, specify P/N 6BL 4VCR for a 6" length, or P/N 12BL 4VCR for a 12" length.

1-5 START-UP/OPERATION

IT IS IMPORTANT TO REMEMBER THAT ALL DIAPHRAGM-VARIABLE CAPACITANCE PRESSURE TRANSDUCERS REQUIRE THE USER TO SET "ZERO" WITH THE SIGNAL CONDITIONER, AFTER SUITABLE WARM-UP AND PUMPING HAVE BEEN ACCOMPLISHED.

THE FOLLOWING PROCEDURE IS PRESENTED AS AN OPTIMUM GUIDE TO ACHIEVING THE FULL DESIGN POTENTIAL OF THE PRECISION 690/698 PRESSURE MEASUREMENT SYSTEM:

698

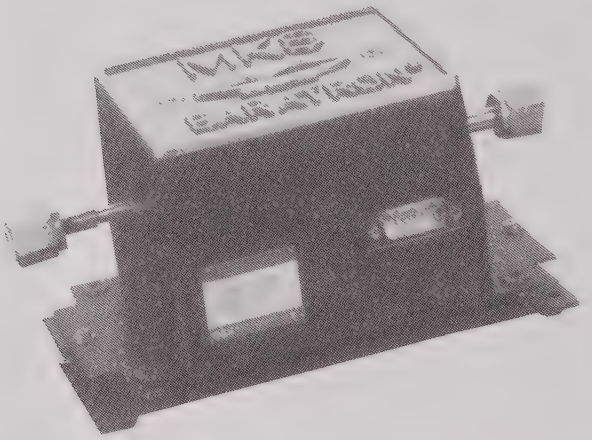

690

1. (690,698): After the sensor has been installed on the system whose pressure is to be measured, it should be connected to its Electronics Unit via the appropriate cable (See Section 1-4F), and power applied.

2. (690,698): A minimum of four (4) hours, and preferably overnight, should be allowed for the heater in the sensor package to thermally stabilize the sensor at control temperature.

3. (690): While waiting for the sensor to reach stable thermal equilibrium, the appropriate vacuum pump/s in the processing System should be engaged, so as to pump down the sensor below its minimum usable resolution.

   (698): While waiting for the sensor to reach stable thermal equilibrium, the appropriate vacuum pump/s in the Processing System should be engaged, in such manner as to provide equal pressure on both sides of the sensor. (This can also be accomplished by cross-porting, i.e., connecting the two ports together).

4. (690,698): After the above warm-up time and pumping requirements have been met, the zero can be properly set.

Each full scale range has different pumping criteria. The following chart summarizes the basic pressures needed prior to setting the "Zero."

SENSOR MODEL NUMBER		RANGE FULL SCALE	HIGHEST PRESSURE FOR PROPER ZERO ADJUST	WARM-UP TIME BEFORE ADJUSTING ZERO
690	HA-0000.1	100 mTorr	$<1 \times 10^{-7}$ Torr	4 Hours Minimum
	HA-0001	1 Torr	$<1 \times 10^{-6}$ Torr	
	HA-00010	10 Torr	$<1 \times 10^{-5}$ Torr	
or	HA-00100	100 Torr	$<1 \times 10^{-4}$ Torr	(It is recommended
	HA-01000	1000 Torr	$<1 \times 10^{-3}$ Torr	all temp-controlled
698	HA-10000	10000 Torr	$<1 \times 10^{-2}$ Torr	transducers be powered continuously)

Note: The best method of zeroing the transducer system is:

First: Center fine pot in the Electronics Unit. This is accomplished by turning the pot to either extreme, noting the voltages at each extreme, and then setting the pot at the half way point.

Next: Adjust zero using the coarse zero pot on the electronics unit.

NOTE: The sensor zero pot is factory set during calibration, and should never be adjusted by the user unless there are suitable transfer or primary standards available to aid in recalibration.

Next: Now Fine Trim the output, using the zero controls on the Electronics Unit. The measurement system is now ready to use.

For reference, the frequency of setting zero will depend on use, variations in ambient temperature, and application. The user will, with experience, gain a feeling for the frequency with which the zero adjustment must be made. For extremely critical measurement of very low pressures, checking the zero more often, and making minor adjustment, will ensure the most accurate measurements attainable with this MKS Baratron^{R} transducer system.

NOTE: The span of the sensor is factory set during the calibration, and should never be adjusted by the user unless there are suitable transfer or primary standards available to aid in recalibration.

If the Zero or Span potentiometers in the sensor head preamplifier are mistakenly adjusted, please contact your nearest MKS Service Center for assistance, and possible instructions to return the instrument to MKS for recalibration.

System Check

The System Check circuit generates a span calibration signal whose precision depends upon the position of the head's zero pot.

1-6 TROUBLESHOOTING

SYMPTOM	CAUSE	REMEDY
CANNOT ZERO		
a. With absolute head.	Pressure not below the reading resolution.	Pump down P_X side.
b. When power first applied.	Head not at operating temperature.	Allow time for stabilization (4 hours minumum).
c. On most sensitive ranges.	Amplifier overload or system noise.	Go back to less sensitive range until on scale and try again and/or try better vibration isolation.
ZERO SHIFT		
a. After applying power.	Sensor temperature shift.	Allow 4 to 6 hours for sensor stabilization. 16 hours for optimum stability.
b. When changing from atmospheric to vacuum operation.	Different outgassing rates for P_X and P_R at vacuum.	Allow time for outgassing completion.
c. When either raising or lowering line.	Leaks in vacuum system.	Check pressure connections at Head and other fittings.
d. Upon turn on of RF power in, for example, a sputtering system. Sudden "negative direction" pressure reading.	Pick up in Sensor Preamplifier.	Replace standard sensor head cable with shielded version or relocate sensor on system or try better grounding.
SYSTEM CHECK		
a. System check voltage different.	Electronics gain has changed.	Check calibration of transducer.

1-7 MAINTENANCE

Generally, nothing needs to be done to maintain the transducer, other than its proper installation and operation. If it fails to operate after doing so for a period of time, return it to MKS for service (obtain from the nearest MKS Service Center an ERA - Equipment Return Authorization - number to expedite handling and assure proper servicing of your transducer). If it fails to operate upon receipt, check the power/signal cable for correct continuity. Also check for shipping damage.

If, after extended use:

1. Measurement goes slowly negative with time. Eventually, one runs out of zero adjustment. This is caused by a reference leak, and requires a new sensor replacement.

2. Measurement goes slowly positive with time. Eventually, one runs out of zero adjustment. This is caused by overpressure, and/or a build-up of contamination in the P_X cavity, which causes the diaphragm to be pushed toward the electrode. Generally, this requires a new sensor replacement.

3. Overrange positive, or negative, signal. This is generally caused by a shorted sensor, or a damaged interconnect cable (sensor to electronics module).

NOTE: If the "zero" output from the transducer is unstable, this is usually caused by the ambient temperature around the sensor or electronics module being too high. The ambient temperature around the sensor must be no higher than 40°C. The ambient temperature around the electronics unit must not exceed 50°C.

2. TRANSDUCER SIMULATOR TYPE HS-1

2-1 DESCRIPTION

The HS-1 Transducer Simulator is used as a test box for checkout and set-up of a precision pressure measurement system (690/698, 270B, 170M-6C). The simulator provides the following functions:

1. A dummy load for, and LED visual signal of, heater supply power.
2. A visual signal of ±15 VDC power supply function.
3. The generation of a zero, 50% FS, and 100% FS signal.
4. Test points for the measurement of the 6 VRMS excitation signal.

Thru its use, one may accomplish the following:

1. Identify a faulty transducer.
2. Identify a faulty cable.
3. Check some of the fundamental functions of the signal conditioner/readout unit.
4. Adjust for transducer-to-signal conditioner cable length.

2-2 HS-1 OPERATING INSTRUCTIONS

SYSTEM CHECKOUT

Disconnect the head cable from the transducer and connect it to the simulator. The red lamp should be ON, indicating that the proper preamp voltage is present at the end of the cable. When the switch is placed in the zero position, a zero signal is developed across the signal input lines. In this position it should be possible to adjust the electronics unit for a stable zero on all ranges. When the switch is placed in the +10V position, the simulator will produce a signal sufficient to produce a stable +10V (full scale) reading on the X1 range.

The HS-1 also contains a resistor to simulate the heater in the sensor. When the heater switch is placed in the REG. position, the heater lamps on the electronics unit will come ON if the supply is working properly. This lamp will not display the same brilliance as it does when attached to a heater due to the higher value of the simulator resistor.

ELECTRONICS UNIT RECALIBRATION

1. Connect a high accuracy AC meter to the jacks on the top of the simulator and measure the amplitude of the oscillator. The proper level is 6.000 VRMS.

2. Place the simulator switch in the zero position, adjust the Null and Full Scale on the indicator and then the zero on all ranges. Then place the range multiplier in the X1 position. Place the simulator switch in the +10V position and adjust the full scale pot on the front of the electronics unit for a reading of +10.00 volts at the output of the electronics unit.

3. Place the simulator switch in the +5V position to check linearity at the 50% point. This should be within 5 mV of 5.00 volts.

OPTIMIZING LONG CABLE OPERATION

When long transducer cables are used in a system, frequently it is necessary to adjust the system gain to optimize system performance which might be degraded due to the cable length. When the simulator is installed on the end of the transducer cable, the system gain is adjusted by using the procedures above. Note that on occasion, the Electronics Unit span adjust may have to be adjusted if the full scale adjustment is insufficient to set full scale.

MKS Worldwide
Customer Support Centers

UNITED STATES

Corporate Headquaters
MKS Instruments, Inc.
Six Shattuck Road
Andover, MA 01810
Phone: (508) 975-2350
(800) 227-8766
Telex: (910) 240-8005
Fax: (508) 975-0093

MKS Instruments, Inc.
789 Grove Road
Suite 111
Richardson, TX 75081
Phone: (214) 231-0173
Fax: (214) 437-4127

MKS Instruments, Inc.
3019 Alvin Devane Boulevard
Suite 210
Austin, TX 78741
Phone: (512) 385-1800
Fax: (512) 385-4411

MKS Instruments, Inc.
3350 Scott Blvd., Bldg. 4
Santa Clara, CA 95054
Phone: (408) 988-4020
Fax: (408) 988-4490

MKS Instruments, Inc.
3189-E Airway Avenue
Costa Mesa, CA 92626
Phone: (714) 641-8555
Fax: (714) 850-0482

NGS Division of
MKS Instruments, Inc.
24 Walpole Park South
Walpole, MA 02081
Phone: (508) 660-1770
(800) 282-1770
Fax: (508) 668-5822

HPS Division of
MKS Instruments, Inc.
5330 Sterling Drive
Boulder, CO 80301
Phone: (303) 449-9861
(800) 345-1967
Fax: (303) 442-6880

CANADA

MKS Instruments, Canada Ltd.
30 Concourse Gate
Nepean, Ontario, Canada K2E7V7
Phone: (613) 723-3386
(800) 267-3551
Fax: (613) 723-9160

FRANCE

MKS Instruments France s.a.
43, Rue de Commandant Rolland
B.P. 41
F-93352 Le Bourget, Cedex, France
Phone: 33(1)48.35.39.39
Telex: 233817 F
Fax: 33(1)48.35.32.52

GERMANY/BENELUX

MKS Instruments
Deutschland GmbH
Schatzbogen 43
D-81829 München, West Germany
Phone: 089/42 00 08-0
Telex: 5 29 997
Fax: 089/42 41 06

UNITED KINGDOM

MKS Instruments, Ltd.
2 St. George Court
Dairyhouse Lane
Altrincham, Cheshire
WA14 5UA, England
Phone: 61-929-5500
Fax: 61-929-5511

ISRAEL

Israel Scientific Instruments, Ltd.
17 Pinhas Street
Ramat-Gan 52306, Israel
Phone: (03) 6772051/2/3/4/5
Fax: (03) 6770808

ITALY

G. Gambetti Kenologia S.N.C.
Via A. Manzoni, 5
20082 Binasco (Milano), Italy
Phone: 9009.30.82
Telex: 315340 KENOL I
Fax: (02) 9052778

JAPAN

MKS Japan, Inc.
Dai-Ichi Shinkoh Bldg., Room 203
No. 28, Yotsuya 4-Chome
Shinjuku-Ku, Tokoyo 160, Japan
Phone: 03-3352-5791
Fax: 03-3352-5790

KOREA

Zeus Co., Ltd.
4th Floor, Zeus Building
3-16, Yangjae-Dong
Seocho-Ku,
Seoul, 137-130 Korea
Phone: (02) 577-3181/6
Telex: K27508 ZEUSCO
Fax: (02) 576-3199

REPUBLIC OF CHINA

Nikko Shoji Taiwan Co., Ltd.
8F-1 No.67, Tzu-Yu Road
Hsinchu, Taiwan
Phone: (035) 424351
Fax: (035) 424352

SINGAPORE

Singapore Electronic & Engineering Ltd.
24 Ang Mo Kio Street 65
Singapore 2056
Phone: (65) 481-8888
Fax: (65) 481-4272